



Can-Dan Mobile Change Table

Under-Table Clearance Guide

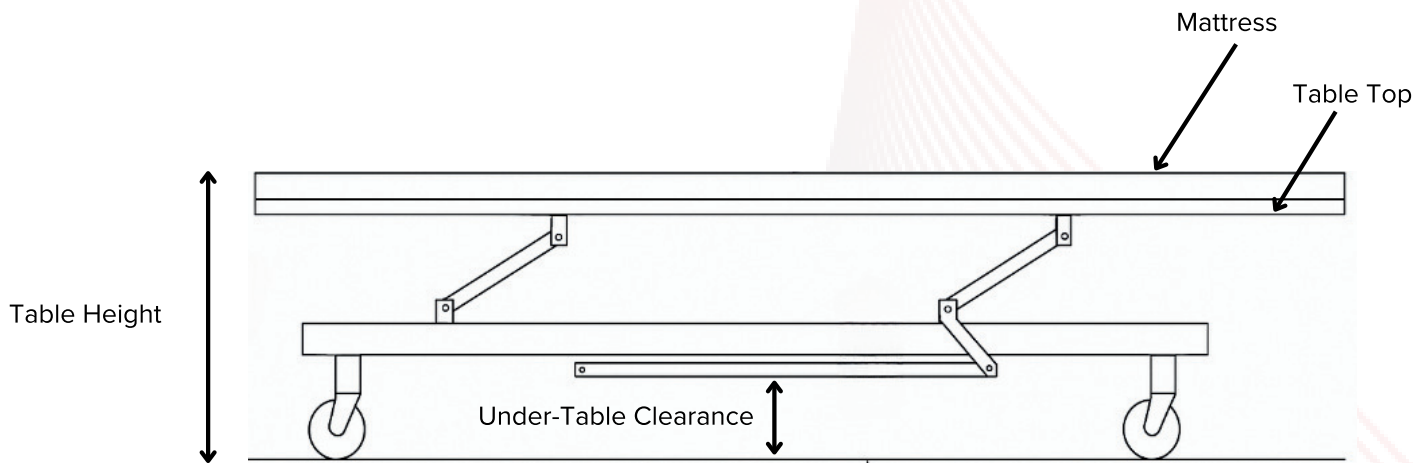


Table Height (floor to top of mattress)	Under Table Clearance
20" - Lowest Height	5.5"
29"	6.25"
34" or higher	7.75"



When using a side rail: If the side rail is down, the table height must be at least 27" to provide a 6" under-table clearance for a patient lift.